


Alcohol / Urine Single Panel Screen 0.04% BAC

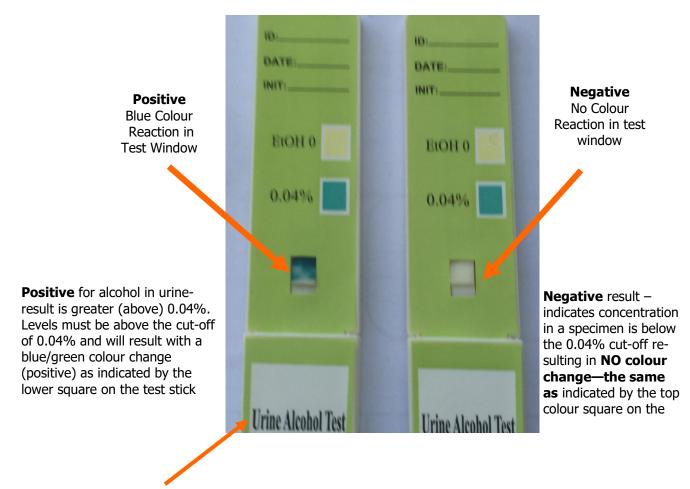

Please remove test cap from test device before inserting into urine sample, once "Test" window has absorbed sufficient sample (2 —30 seconds), remove device from specimen, re-cap and lie on a flat surface.

Read colour results at 5 minutes maximum time lapse.

0.04% (BAC) = 200ng/mL BrAC

0.08% BAC = 400ng/mL BrAC 0.05% BAC = 200ng/mL BrAC

Drugchek NZ: W: www.drugchek.co.nz E: sales@drugchek.co.nz T 09 849 4512