



# InnoScreen Rapid

**6 Panel Drug Screen  
Verified to  
AS/NZ 4308:2008**



**Verified to Appendix B of the AS/NZ4308:2008 Drug Testing Standard, InnoScreen Rapid Tilt Cup is based on the same principle as the Proscreen cup. Collector screws the lid on and the test is activated by tilting the cup onto the legs of the lid.**

**Accurate and cost effective 6 panel screening- providing accurate, rapid results in minutes Simply collect sample, screw lid on, read temperature before tilting to activate results for integrity screens and test results**

## CONVENIENCE

- Tests for the six drugs of abuse as per AS/NZ4308:2008 requirements/cut-offs
- Incorporates collection and testing
- Temperature strip on cup
- Adulterant strips included to defeat specimen adulteration
- Simple procedure, collect sample read test in 5 minutes, no timing required

## PERFORMANCE

- Each test has procedural control built in Colloidal gold technology
- >99% correlation to GC/MS at 97.5% confidence level
- Tested for cross-reactivity against 500 drugs
- **AS/NZ Standard 4308:2008 cut-offs**
- **Verified under Appendix B to the AS/NZ 4308:2008 Standard**

## CUT-OFF LEVELS

- Cut-off levels to AS/NZ Standard 4308:2008 for immunoassay testing : -  
Amphetamines/Methamphetamines 300ng/ml,  
Benzodiazepines 200ng/ml, Cocaine 300ng/ml  
Opiates 300ng/ml, THC (Marijuana) 50ng/ml

## AMP

amphetamines 300ng/ml

## BZO

benzodiazepines 200ng/ml

## COC

cocaine 300ng/ml

## METH

methamphetamine 300ng/ml

## OPI

opiates 300ng/ml

## THC

marijuana 50ng/ml

## Plus 6 Integrity Tests

- **Oxidants**
- **Specific Gravity**
- **pH (alkaline & acidity)**
- **Glutaraldehyde**
- **Nitrites**
- **Creatinine**
-

# Innoscreen Rapid

**6 Panel Drug Screen  
Verified to  
AS/NZ 4308:2008**



Innoscreen Rapid 6 panel drug screen is a rapid urine screening immunoassay device for the detection of the drugs of abuse in urine. Easy to use, accurate and cost effective with results available in minutes


## Easy to Use

Collector gives sealed specimen cup to donor


1. Donor provides specimen returning sample to collector .
2. Collector opens foil pouch and removes lid of device—screw onto the cup
3. Collector checks temperature strip is in range (32-38C)
4. Collector then tilts to cup onto the legs of the lid
5. View results, checking integrity tests with colour card provided
6. Interpret drug screening results:
  - Control line (**C**) should appear in all test windows.
  - A second line (**T**) should then appear for all test windows (**negative**)



- A positive/**non-negative** is indicated by the **ABSENCE** of a test line below the corresponding drug
- line intensity (colour) is **NOT** important

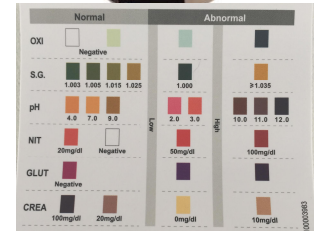

## Reading Results

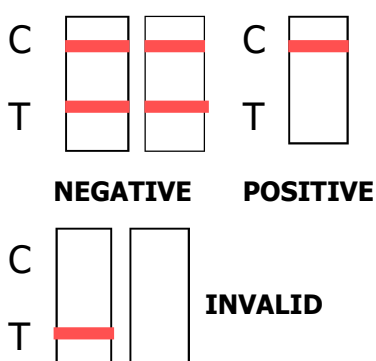

C = Control  
T = Test

All positive results are presumptive & should be **confirmed by lab GC/MS (Gas Chromatograph/Mass Spectrometry)**

Line Intensity is **NOT** important

- Negative results can be read as soon as they appear
- Read non-negative results at 5 minutes
- Line intensity is **NOT** important
- All non-negative results are presumptive and should be confirmed by GC/MS (Gas Chromatograph/Mass Spectrometry)

Negative = 2 lines in each window  
NON Negative = only a Control line visible in window